

HRE031-P02

Room:Convention Hall

Time:May 24 16:15-18:45

An Experimental Equipment for Permeability Using Super-Critical CO₂

Masaki Ono^{1*}, Kohichi Hosoda¹, Hiroshi Kameya², Yotsuo Kamidozono¹, Junya Takeshima², Hiroyuki Azuma², Shinichi Hiramatsu²

¹OYO Corporation, OYO Core Lab, ²OYO Corporation, OYO Energy Division

To estimate fluid flow in underground during CO₂ geological sequestration, the properties of the two phase flow such as relative permeability are necessary. There are essentially three means by which relative-permeability data can be obtained. They are (1) direct measurement in a laboratory, (2) calculation by capillary pressure data and (3) calculation from field-performance data. In CO₂ geological sequestration, however, residual water saturation which means the non displaced portion of water by CO₂, is very important and this value can't be estimated from capillary pressure. Also field-performance data can't be acquired except demonstrations of CO₂ geological sequestration or EOR gas storage in oil-fields. So we think that direct measurement of relative permeability in laboratory is necessary for site assessment.

There are two kinds of test methods to determine relative permeability directly by laboratory experiment. One is the steady-state method and the other is unsteady-state or displacement method. In the steady-state method, a specimen is initially saturated with water. Two fluids are introduced at predetermined fluid ratio and are flowed through the specimen until the produced ratio is equal to the injected ratio. At this time, the specimen is considered to be in steady-state flow condition and the existing saturation of the specimen is considered to be stable. The injected ratio is increased, removing more of water, until once again the specimen be in steady-state flow condition. This process has to be continually repeated until complete relative permeability curve is obtained. So this method is rather involved and time consuming.

On the other hand, the displacement method is rather simple and fast. A specimen is saturated with water, and only gas (CO₂) is injected into the specimen. Differ from the steady-state method, only one fluid is entering the core, and two fluids are leaving.

Figure.1 shows the schematic view of relative permeability test apparatus. Using this apparatus, the test samples can be flooded with CO₂ in super-critical condition. CO₂ is pressurized in the injection pump, then flow into the sample inside the core holder which is set in the incubator at desired temperature. The maximum pressure capacity of the core holder is 50MPa, and the maximum pressure capacity of fluid tubing system is 25MPa. So this apparatus can reproduce the pressure condition of underground in the depth of 2000m.

In the process of relative permeability test, two kinds of fluids flow out from a core sample. In the displacement method, cumulative volume of each fluid must be measured individually for the calculation of relative permeability and saturation of the sample. Two fluids separate in a separator on account of the effect of their density difference and one fluid (usually displacing fluid) flows out, the other (displaced fluid) remains in the separator. The total outflow volume can be evaluated from the amount of the back-pressure pump during the experiment, so the cumulative volume of each fluid can be calculated using data of water level change in the separator. There are some ways to measure water level in a separator. One is the visual measurement through a window of separator. The other is indirect measurement using differential pressure transducer or electric capacitance. We adopted electric capacitance because installing a window to the separator is difficult in compliance with regulation.

In steady-state method, the main experimental problem is accurate measurement of saturation. In many case, the saturation is measured directly by measuring sample weight or estimated by in-situ measurement using resistivity, NMR, micro wave absorption or X-ray CT scanning. These are the technique that we must add with our apparatus if we conduct the steady-state relative permeability test.

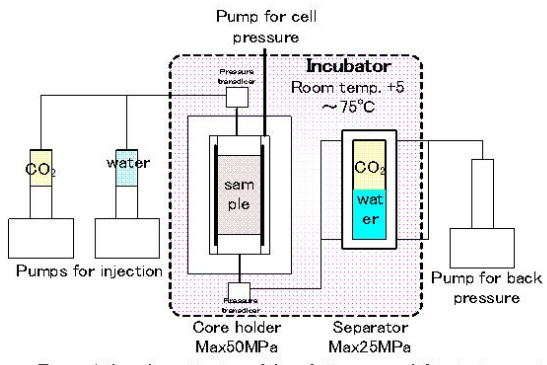


Figure 1 the schematic view of the relative permeability test apparatus

Keywords: CCS, Two Phase Flow, Relative permeability, laboratory experiment